

INTRAOCULAR LENS


ARTIS[®] PLE

HYDROPHOBIC ACRYLIC



Micro-incision

Preloaded

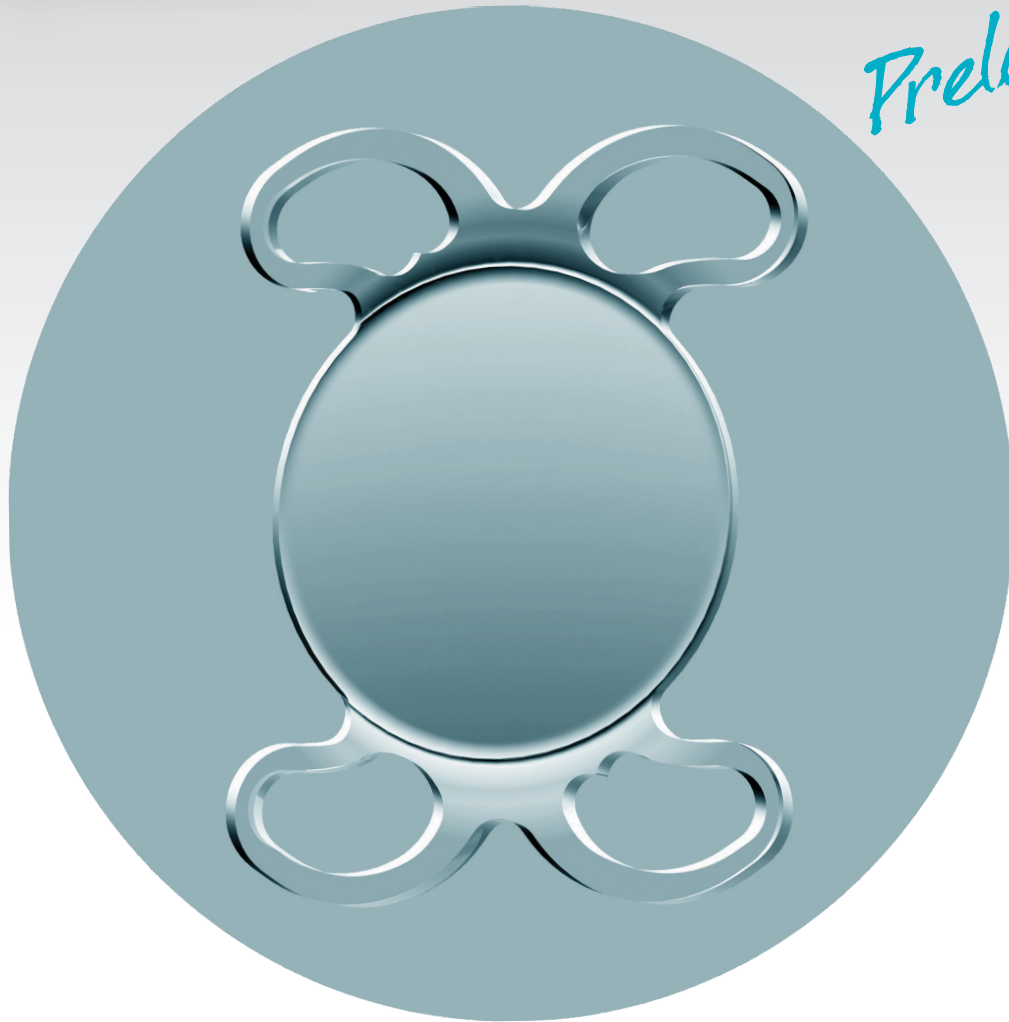

Made in France

CE 0459



Ophthalmologic
surgery

Cristalens

DESIGNATION	TECHNICAL SPECIFICATIONS
Lens Type	For implantation in the capsular bag
Optic diameter	6.15 mm (from oD to +9.5D) 6.00 mm (from +10D to +25D) 5.80 mm (from +25.5D to +35D)
Overall diameter	11.00 mm (from oD to +9.5D) 10.79 mm (from +10D to +25D) 10.50 mm (from +25.5D to +35D)
Design	One piece square edge on 360°
Optic design	Aspherical on the posterior surface Compensation of corneal aberrations
Angulation	5°
Material	Hydrophobic acrylic for micro-incision
Dioptric powers	From oD to +35D by 0.5D
Estimated A-Constant (SRK-T)	119.3 Ultrasound biometry 119.7 Interference laser biometry
Suggested Anterior Chamber Depth (ACD)	5.77 mm Ultrasound biometry 6.03 mm Interference laser biometry
Refractive index	1.54
Sterilization	Ethylene oxide
Recommended incision size	< 2.2 mm oval shape

13/02/2014 DOC_10_PHOBIC



Ophthalmologic
surgery
Cristalens

12 allée Rosa Luxemburg - BP 50240 Eragny
95615 Cergy Pontoise cedex - France

Tél : + 33 (0) 1 34 32 30 50 - Fax : + 33 (0) 1 34 32 30 60



Cristalens Industrie

4 rue Louis de Broglie - 22300 Lannion - France

Tél : + 33 (0) 2 96 48 92 92 - Fax : + 33 (0) 2 96 48 97 87

www.cristalens.fr

Cristalens