


INTRAOCULAR LENS

CLARÉ®

Hydrophilic acrylic
Micro incision 1.8 mm

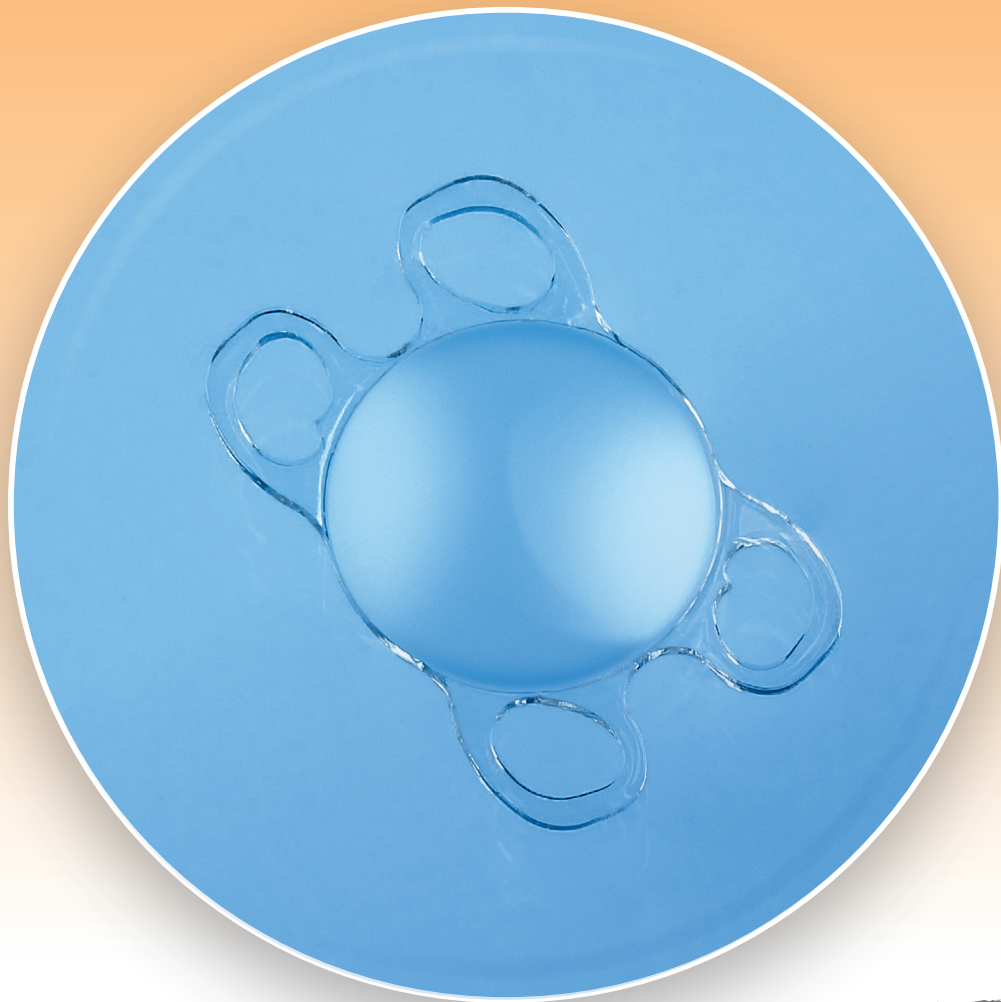

Made in France
CE 0459


Ophthalmologic
surgery


Cristalens

INTRAOCULAR LENS

CLARÉ®

TECHNICAL SPECIFICATIONS

DESIGNATION	TECHNICAL SPECIFICATIONS
Lens type	For implantation in the capsular bag
Optic diameter	6.0 mm from + 10.0 D to + 24.5 D 5.7 mm from + 25.0 D to + 30.0 D
Overall diameter	11.00 mm from + 10.0 D to + 14.5 D 10.75 mm from + 15.0 D to + 24.5 D 10.50 mm from + 25.0 D to + 30.0 D
Design	One piece with square edge 360°
Optic design	Aspheric on the posterior surface, Compensation of corneal aberration
Angulation	8°
Material	Hydrophilic Acrylic 25 %
Dioptric powers	From + 10.0 D to 30.0 D - from + 10.0 D to 14.0 D by + 1 D - from + 14.5 D to 25.5 D by + 0.5 D - from + 26.0 D to 30.0 D by + 1 D Other diopter available on request
Estimated A-Constant (SRK-T)	118.0 Ultrasound biometry 118.5 Interference laser biometry
Suggested anterior chamber depth (ACD)	4.96 mm Ultrasound biometry 5.25 mm Interference laser biometry
Refractive index	1.46
Sterilization	Steam sterilization
Recommended incision size	1.8 mm



Ophthalmologic
surgery
Cristalens

12 allée Rosa Luxemburg - BP 50240 Éragny
95615 Cergy Pontoise cedex - France
Tél : + 33 (0)1 34 32 30 50 - Fax : + 33 (0)1 34 32 30 60

Cristalens Industrie
4 rue Louis de Broglie - 22300 Lannion - France
Tél : + 33 (0)2 96 48 92 92 - Fax : + 33 (0)2 96 48 97 87
www.cristalens.fr

Cristalens